


# Masimo SET vs. Nellcor N-600



This study measured the occurrence rate of missed true events during 40 low blood oxygen episodes and false alarms during 120 fully oxygenated episodes, both during conditions of motion.

Nitin Shah, M.D., Laverne Estanol, M.S. *Anesthesiology*, 2006 Long Beach VA Medical Center, UC Irvine Medical Center, Long Beach, California  
Comparison of Three New Generation Pulse Oximeters During Motion & Low Perfusion in Volunteers

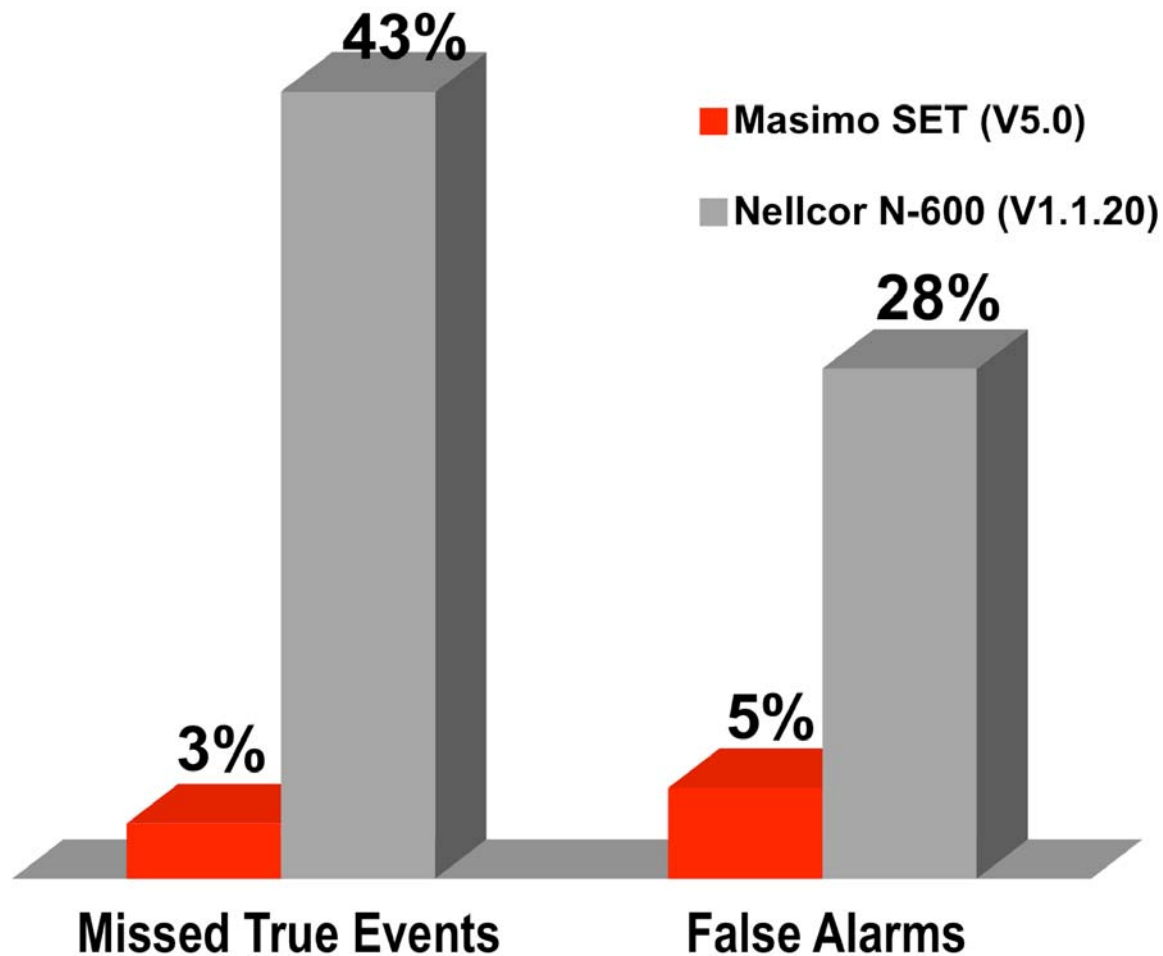